



(11) **EP 2 034 347 A1**

(12) **EUROPEAN PATENT APPLICATION**
published in accordance with Art. 153(4) EPC

(43) Date of publication:
11.03.2009 Bulletin 2009/11

(51) Int Cl.:
G02B 21/00 (2006.01)

(21) Application number: **07743988.3**

(86) International application number:
PCT/JP2007/060554

(22) Date of filing: **23.05.2007**

(87) International publication number:
WO 2007/136100 (29.11.2007 Gazette 2007/48)

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IS IT LI LT LU LV MC MT NL PL PT RO SE SI SK TR
Designated Extension States:
AL BA HR MK RS

(72) Inventors:
• **NISHIZAKA, Takayuki**
Tokyo 171-0031 (JP)
• **YASUDA, Ryohei**
Chapel Hill, North Carolina 27514 (US)

(30) Priority: **24.05.2006 JP 2006144050**

(74) Representative: **De Groote, Christophe et al**
Pecher Consultants
Rue du Bosquet 7
1348 Louvain-la-Neuve (BE)

(71) Applicant: **Japan Science and Technology Agency**
Kawaguchi-shi
Saitama 332-0012 (JP)

(54) **DARK FIELD MICROSCOPE AND ITS ADJUSTING METHOD**

(57) Dark field microscope comprising a light source for emitting illumination light, a light collecting optical system including a light collecting side condenser lens for collecting the illumination light from the light source to illuminate an observation sample, and an image forming optical system comprising an objective lens for receiving scattered light from the observation sample to form a magnified image of the sample. The light collecting side condenser lens is a long focal distance lens, and a light shielding member for shielding the illumination light is provided at an image forming center on a back focal plane in the image forming optical system.

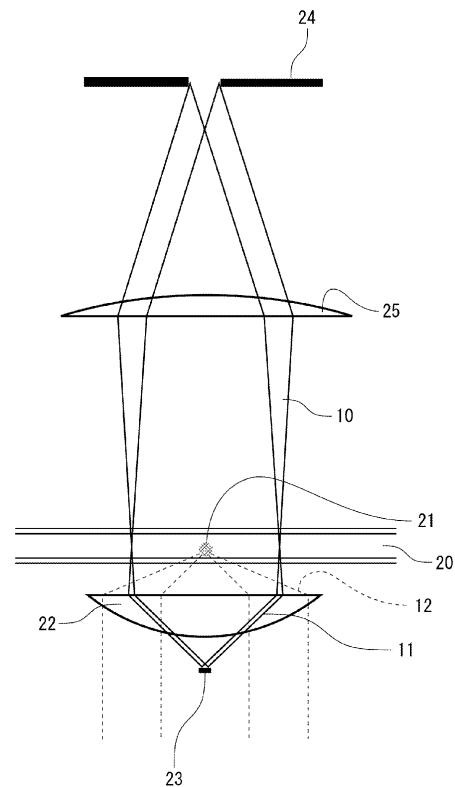


Fig. 2

EP 2 034 347 A1

Description

[Field of the invention]

5 **[0001]** The present invention relates to a dark field microscope and a method for adjusting its optical axis.

[State of the art]

10 **[0002]** Dark field microscopes are well known in the state of the art. Such known microscopes include a light source for emitting illumination light, a light collecting optical system including a light collecting side condenser lens for collecting the illumination light from the light source to illuminate an observation sample, and an image forming optical system including an objective lens for receiving scattered light from the observation sample to form a magnified image of the sample.

[0003] Fig. 1 is an explanatory diagram illustrating a principle of a known dark field microscope.

15 **[0004]** Light from a light source is illuminated on an observation sample (21) located in a flow cell (20), through a light collecting side condenser lens having a high numerical aperture and yielding a hollow cone illumination light (10) pattern. The illumination light (10) is scattered by the sample (21) to form scattered light (12). However, the illumination light (11) itself is shielded by an aperture diaphragm (23) present within an objective lens (22). As a result, only the scattered light (12) is emitted from the objective lens (22, 23). By collecting the scattered light (12) on an imaging area of a camera, a dark field image of the sample (21) can be obtained.

20 **[0005]** Light is scattered even by a particle or a structure smaller in size than a wavelength thereof, and therefore, when a dark field microscope is used, even an object having a size equal to or smaller than a wavelength of visible light can be observed.

25 For example, a microtubule having a diameter as small as approximately 24 nm, becomes visible by a dark field microscope having a mercury lamp as a light source.

[0006] The dark field microscope has additional advantages, such as, for example: the device in itself and its operation are relatively simple, a high contrast image can be obtained, a raw sample can be observed without preprocessing, supermolecular movement and morphology change can be dynamically observed, and so on.

30 **[0007]** State of the art dark field microscopes are known from Patent documents 1 to 4.

Patent document 1: Japanese Unexamined Patent Publication No. H09-297266, "Microscope"

Patent document 2: Japanese Unexamined Patent Publication No. H09-15507, "Dark field microscope"

Patent document 3: Japanese Unexamined Patent Publication No. H08-122651, "Transmission dark field microscope"

35 Patent document 4: Japanese Unexamined Patent Publication No. H05-346532, "Automatic focusing device of microscope and dark field microscope"

40 Patent document 1 relates to an illumination system capable of easily switching between a bright field and a dark field. Patent document 2 relates to a configuration capable of observing only a target micro object without reducing a resolution.

Patent document 3 relates to a configuration capable of observing an extremely small object such as a flagellum of a living bacterium.

45 Patent document 4 relates to high speed processable automatic focusing and increase in brightness in the dark field microscope.

[0008] Such known dark field microscopes require the presence of an aperture diaphragm (23) within the objective lens (22), and are also subject to the constraint that the light collecting side condenser lens should have a high numerical aperture.

50 **[0009]** If illumination can be provided through a long focal distance condenser lens having a low numerical aperture, additional space will be available above the flow cell (20). This results among others in a wider application range for experimental observation.

[0010] However, a dark field microscope capable of realizing this has been absent.

[Summary of the invention]

55

[Problem to be solved by the invention]

[0011] It is therefore an object of the present invention to provide a dark field microscope capable of providing illumi-

nation even through a long focal distance condenser lens having a low numerical aperture, and without the need for an aperture diaphragm within an objective lens, and a method for effectively adjusting its optical axis.

[Means adapted to solve the Problems]

5
[0012] In order to accomplish the above object, a dark field microscope according to the present invention comprises a light source for emitting illumination light, a light collecting optical system including a light collecting side condenser lens for collecting the illumination light from the light source to illuminate an observation sample, and an image forming optical system including an objective lens for receiving scattered light from the observation sample to form a magnified image of the sample, wherein the light collecting side condenser lens is a long focal distance lens, and a light shielding member for shielding the illumination light is provided at an image forming center of a back focal plane in the image forming optical system.

10
[0013] Preferably, in the image forming optical system according to the invention, the light shielding member is disposed at a position of a conjugate image of the back focal plane formed by forming a secondary image from a primary image. This configuration enables the light shielding member to be disposed outside the objective lens, which contributes to a simplification of the configuration.

15
[0014] As the light shielding member disposed at the image forming center of the conjugate image of the back focal plane, a light shielding plate having a diameter of $\phi_e = \phi \cdot f_1 / L$ (ϕ is a diameter of an area to be shielded on the back focal plane; f_1 is a focal distance of the lens for forming the conjugate image of the back focal plane; and L is a focal distance of a second objective lens) may be used to contribute to the effective light shielding.

20
[0015] The image forming optical system for forming the secondary image from the primary image may include a plurality of lenses, and, under a condition that a total focal distance of lenses for forming the conjugate image of the back focal plane among the plurality of lenses is $f_t = L \cdot \phi_e / \phi$ (L is a focal distance of a second objective lens; ϕ_e is a diameter of the light shielding member; and ϕ is a diameter of an area to be shielded on the back focal plane), a numerical aperture may be adjusted, yet keeping a size of the light shielding member constant.

25
[0016] Also, a mirror may be provided between the primary image and the secondary image to contribute to a dual port configuration.

30
[0017] In a configuration including the dark field microscope as described above and a camera for receiving an image formed by said dark field microscope, optical axis adjustment may be performed by adjusting a focal point of an eyepiece lens to thereby focus on the observation sample, adjusting a position of the light collecting side condenser lens to thereby provide Koehler illumination, adjusting a position of the image forming side lens to thereby focus the observation sample on an imaging area, adjusting a diaphragm for a primary imaging plane and a position of the mirror to thereby match a field center with a center of the camera, and adjusting a position of the light shielding member in an optical axis direction to thereby set it at a position where background light is reduced to a minimum.

35
[0018] In this case, the position of the light shielding member may be adjusted in a direction perpendicular to the optical axis, for example with a micrometer.

40
[0019] A contribution to obtaining a desired contrast may be made further by minimizing a field diaphragm on the light collecting side condenser lens, adjusting a black level with preventing the light from entering the camera, to thereby set a value of the level not to take a negative value, switching the light to a camera side, and adjusting an aperture diaphragm with the observation sample being focused on, to thereby set the aperture diaphragm at a position where the image becomes dark, and adjusting light intensity and the aperture diaphragm to thereby increase an amount of light and reduce a numerical aperture.

45
[0020] The image may be made more visible by adjusting the black level to thereby optimize a background of the observation sample.

[0021] A preferred brightness may be obtained by adjusting the light intensity to thereby increase an amount of the scattered light from the observation sample.

[Effect of the invention]

50
[0022] According to the dark field microscope of the present invention, because the light shielding member is provided at the image forming center of the back focal plane in the image forming optical system, an aperture becomes unnecessary for the objective lens. Moreover, illumination can be provided through a long focal distance condenser lens having a low numerical aperture. As a result, more space is available at one side of the observation sample, and hence the application range of experimental observations is enlarged.

55
[0023] Also, according to the dark field microscope adjusting method of the present invention, the optical axis can be accurately adjusted with a conventional low-cost optical system, microscope, camera, and the like.

[Brief description of the drawings]

[0024] These and further aspects of the invention will be explained in greater detail by way of example and with reference to the accompanying drawings, in which :

5

Fig. 1 is an explanatory diagram illustrating a principle of a known general dark field microscope.

Fig. 2 is an explanatory diagram illustrating a principle of a dark field microscope according to the present invention.

10

Fig. 3 is a profile for a case where a bead was observed.

Fig. 4 is a diagram for a case where gliding motion of a bacterium was photographed.

15

[0025] The figures are not drawn to scale. Generally, identical components are denoted by the same reference numerals in the figures.

[Detailed description of preferred embodiments]

20

[0026] Note that the exemplary embodiments described hereinafter can be appropriately changed in design without departing from the scope of the present invention.

[0027] The present inventor has reviewed the nature of a dark field microscope to thereby obtain a principle of the present invention as follows : the nature of the dark field microscope is considered as means adapted to shield the illumination light (11) with a particular optical member in order to image only the scattered light (12).

25

[0028] As illustrated in Fig. 1, in the known techniques, the reason why the illumination light (11) is annular in section is that the shielding can be effectively performed by a diaphragm. That is, a configuration of illumination is determined by the shielding means.

[0029] On the other hand, assume that the illumination system can not be freely chosen and that, for example, only a long focal distance condenser lens may be used. In such a case, by changing a shielding configuration, a function as a dark field microscope becomes possible.

30

[0030] Fig. 2 is an explanatory diagram illustrating the principle of a dark field microscope according to the present invention.

[0031] Light from a light source passes through an aperture diaphragm (24), and then illumination light (10) is illuminated on a sample (21) in a flow cell (20) only through a low numerical aperture area of a long focal distance light collecting side condenser lens (25).

35

[0032] Such illumination method should be chosen when, for example, a magnetic tweezer or a solution exchange system is being used.

[0033] The illumination light is scattered by the sample (21). However, an image forming center of the illumination light itself (11) is shielded by a light shielding member (23) disposed on a back focal plane of an objective lens (22). For this reason, only scattered light (12) emitted from the objective lens (12) is collected on an imaging area of a camera, so that a dark field image of the sample (21) can be obtained.

40

[0034] For the light-shielding member (23), a transparent vapour-deposited optical component affixed in the centre of a light reflecting material, such as aluminium, may be used. It is also possible to use light absorbing material, such as suede, to which a glass plate is affixed in a central position.

[0035] A light flux of an optical system is defined by field and aperture diaphragms. The field diaphragm defines an image size, whereas the aperture diaphragm defines a diameter of the light flux, i.e., a numerical aperture.

45

[0036] A value of the numerical aperture is defined for each objective lens. In addition, when observing with the eye through an eyepiece lens, an image of an aperture diaphragm through a lens before the aperture diaphragm is an entrance pupil and an image of an aperture diaphragm through a lens after the aperture diaphragm is an exit pupil, and the aperture diaphragm, the entrance pupil, and the exit pupil are respectively in conjugate relations.

50

[0037] Also, a light flux from a sample plane is formed of lines connected between respective points of the sample plane and the entrance pupil, whereas a light flux toward an image plane is formed of lines connected between the exit pupil and respective points of the image plane.

[0038] In general, a numerical aperture (NA) is given by the following expression:

55

$$NA = n \cdot \sin\theta \quad (\text{Expression 1})$$

(n : refractive index, θ : illuminating angle of light)

[0039] The numerical aperture serves as an indicator for recognizing an angle at which the illumination light (10) is illuminated on the sample (21). As the illumination angle becomes steeper, a resolution of an image becomes higher. Because a scattering angle of light increases as a particle size decreases, light picked up by a higher numerical aperture area contains more high frequency components of the image, and therefore a finer structure can be observed. Thus, the numerical aperture is an important quantity for determining the resolution of an image.

[0040] Also, the reason why a characteristic of the objective lens (22) is expressed by the numerical aperture instead of an actual illumination angle θ is also obvious considering Snell's law. Even if light is refracted at an interface between different media, a value of $n \cdot \sin\theta$ is conserved, and therefore the use of the numerical aperture is more effective than the actual illumination angle θ itself.

[0041] A diameter ϕ of a pupil met by some numerical aperture in the objective lens (22) (infinity system) can be approximated by the following expression:

$$\phi = 2 \cdot \text{NA} \cdot L / M \quad (\text{Expression 2})$$

(L: focal distance of a second objective lens, M: magnification of the objective lens)

[0042] The pupil can be considered as a size of a back focal plane. The back focal plane is an area where parallel light is collected when the light passes through an image plane. Also, if an ideal point light source is present on the image plane, a diameter of light expanding from the light source with some numerical aperture can be here considered as a diameter of the pupil.

[0043] Note that, on the back focal plane of the objective lens (22), the numerical aperture does not mean an angle but means a radius. On the sample plane, it images the angle, whereas on the back focal plane, it corresponds to a circular ring whose area can be calculated from Expression 2. Also, if the sample is illuminated through a condenser lens (25), a corresponding numerical aperture is the same as in the case of the objective lens (22).

[0044] In Fig. 2, the light shielding member (23) is disposed on the back focal plane of the objective lens (22). However, if the secondary image is created from the primary image with a lens being disposed behind a camera port, a conjugate image of the back focal plane can be formed between them. The light shielding member may therefore be disposed at the position of the conjugate image.

[0045] A diameter ϕ_e of the light shielding member for this case is given by the following expression:

$$\phi_e = \phi \cdot f_1 / L \quad (\text{Expression 3})$$

(ϕ : diameter of an area to be shielded on the back focal plane, f_1 : focal distance of the lens forming the conjugate image of the back focal plane, L: focal distance of the second objective lens)

[0046] By substituting Expression (3) into Expression (2), following Expression (4) can be obtained :

$$\text{NA} = \phi_e \cdot M / 2f_1 \quad (\text{Expression 4})$$

[0047] In Expression (4), L is absent, and therefore it turns out that this expression is effective regardless of a microscope type.

[0048] In addition, when observing with the eye through an eyepiece lens, an exit pupil of the eyepiece lens corresponds to a pupil plane referred to as an eye point. Similarly to the relationship relating to the image plane, an exit pupil is relayed as an entrance pupil of a subsequent lens with the pupil planes being related to each other. For this reason, in a lens system after the objective lens (22), a position of a pupil cannot be uniquely defined. A distance between the objective lens (22) and a lens barrel may be changed, and therefore if a plurality of optical systems are connected, pupil matching is required.

[0049] The present invention can also be applied to dark field illumination with a laser as a light source, for example in case particularly strong light illumination is required for high speed photography.

[0050] In the known systems (for example : Yasuda, R., Noji, H., Yoshida, M., Kinoshita, K., Jr. & Itoh, H. - Resolution of distinct rotational substeps by submillisecond kinetic analysis of F1-ATPase. Nature 410, 898-904 (2001)), the laser beam in a dark field microscope is obliquely incident with respect to the sample plane in order to avoid loss of light intensity.

[0051] According to the present invention, laser light is incident perpendicularly with respect to a sample plane, as

with an arc type light source. The illumination light then forms a point image on a back focal plane, and shielding it with the light shielding member (23) at the center results in the dark field illumination. This illumination is more isotropic than the oblique illumination, and therefore has an advantage of being able to obtain a more uniform image.

5 [Example]

[0052] A dark field microscope based on the principle of the present invention was assembled with commercially available optical components manufactured by a plurality of optical equipment manufacturers.

10 **[0053]** As a lens for forming a secondary image from a primary image, a combination of $f_1 = 60$ mm and $f_2 = 150$ mm was used to observe dust on a glass surface, and a good result was obtained, similar to that obtainable with a conventional dark field microscope. However, there remains a problem that in case a halogen wavelength band was narrowed with a filter, a sufficient amount of light could not be obtained.

15 **[0054]** As a numerical aperture of a condenser lens increases, the amount of illumination light increases, and therefore a numerical aperture that should be light shielded also increases. However, an amount of light illuminating the sample (21) also increases. If an objective lens (22) having a numerical aperture of 1,45 is used, it is considered that a sufficient amount of scattered light (12) can be obtained from the sample (21) even if the center of it is further shielded by an amount of numerical aperture of 0,25.

[0055] If a light shielding plate is used as the light shielding member (23), it may be freely configured and replaced by any of various sized ones.

20 **[0056]** Instead of variously configuring a diameter of the light shielding member (23), a configuration may be made such that an imaging lens closer to the primary image is replaced, and the focal distance f_1 of it is variable. As is obvious from Expression (4), if f_1 is decreased, a numerical aperture of the light shielding plate for the entire optical system can be increased.

25 **[0057]** Also, under the condition that the image forming side optical system for forming the secondary image from the primary image includes a plurality of lenses, and a total focal distance of lenses for forming a conjugate image of a back focal plane among the plurality of lenses is adapted to be $f_t = L \cdot \phi_e / \phi$, the numerical aperture may be adjusted with the size of the light shielding member (23) being constant.

[0058] If a dual port TV adaptor or the like is annexed, it is preferable to place a mirror between the primary image and the secondary image, and to position the conjugate image of the back focal plane also before the mirror.

30 **[0059]** The light shielded numerical aperture, i.e., a numerical aperture used for the illumination was set to 0,375 with f_1 set to 40 mm. Compared with the case of $f_1 = 60$ mm, the light intensity is increased by a factor of $(60 / 40)^2 = 2,25$. However, the area of the objective lens is reduced by a factor of $(1,45 - 0,375 / 1,45 - 0,25)^2 = 0,80$, due to the light shielding. As a result, the light intensity is increased by a factor of approximately 1,8 .

[0060] Fig. 3 is a profile for a case where a bead having a diameter of 0,2 μm was observed.

35 **[0061]** The sample bead is made of polystyrene, and bonded to a glass surface.

[0062] As a result of the observation under a condition that the lens for forming the secondary image from the primary image was set to have $f_1 = 40$ mm and $f_2 = 150$ mm, and the diameter of the light shielding plate was $\phi = 500$ mm, the bead was observed with sufficient brightness. In spite of a state where a gain of a CCD was maximized, and a dichroic mirror and an emission filter were attached for fluorescence observation, it turns out that the single piece of bead can be observed with sufficient intensity as illustrated in the diagram.

[0063] Fig. 4 is a diagram for a case where gliding motion of a bacterium was actually photographed.

[0064] One individual piece of Mycoplasma Mobile, which is motile bacteria, was observed, and as a result, it turns out that the gliding motion can be observed without any problem.

40 **[0065]** The bacteria (30) and (31) moved from start positions illustrated in Fig. 4 (A) along lines (31) and (31') indicated by arrows, and then reached end positions illustrated in Fig. 4 (B).

45 **[0066]** Regarding optical axis adjustment, a following procedure is preferable:

(1) Focus on a sample.

50 (2) Adjust xyz coordinates of the condenser lens so as to achieve Koehler illumination. Note that the Koehler illumination requires a condenser lens having a numerical aperture which is sufficient for observation, an illumination system in which a light source image can be projected on a focal plane of the condenser lens, and the field diaphragm can be properly imaged on the sample plane and narrowed down to a necessary part.

(3) Switch the light to a camera side, and move a position of the condenser lens f_1 to focus the sample on the imaging area. This causes focuses of the eyepiece lens and the camera to be matched.

55 (4) Narrow the diaphragm for a primary imaging plane to adjust the mirror such that the center of a field is matched with that of the camera.

(5) Move the light shielding plate in an optical axis direction to set it at a position where the light illuminating the camera becomes darkest. Preferably, it is performed while moving the shielding plate in x, y directions with a

micrometer.

Subsequently, as fine adjustment, a condition for obtaining an optimum image is found out by changing a setting of an aperture diaphragm, an amount of light, and a black level of the camera.

(6) Adjust the black level of the camera not to take a negative value with the field diaphragm on the condenser lens being set to a minimum in order to prevent the light from entering the camera.

(7) Switch the light to the camera side; gradually narrow down the aperture diaphragm with the sample being focused on; and set the aperture diaphragm at a position where an entire screen suddenly darkens. In this state, a numerical aperture light shielded by the central light shielding plate and that of the condenser lens are matched.

(8) Increase intensity of the light, and when the entire screen is about to be saturated, further narrow down the numerical aperture. By alternately repeating these two operations, an optimum contrast can be obtained.

(9) If the black level is adjusted such that a background reaches approximately 10 in 8 bits, the image becomes more visible. If necessary, further increase the amount of light while monitoring brightness.

[Industrial applicability]

[0067] According to the dark field microscope based on the new principle of the present invention, with advantages of a conventional optical system, microscope, camera, and the like being taken, a diaphragm for an objective lens becomes unnecessary, and illumination can be achieved even with a long focal distance condenser lens having a low numerical aperture.

[0068] Along with this, a space can be ensured above an observation sample plane, and therefore an application range of experimental observation is expanded. This is particularly effective when using a magnetic tweezer or a solution exchange system that should employ such illumination method.

[0069] The dark field microscope has wide ranging applications in industrial fields such as an IC (Integrated Circuit) pattern inspection, and is industrially very useful.

Claims

1. A dark field microscope comprising a light source for emitting illumination light (10, 11), a light collecting optical system including a light collecting side condenser lens (25) for collecting the illumination light (10) from the light source to illuminate an observation sample (21), an image forming optical system including an objective lens (22) for receiving scattered light (12) from the observation sample (21) to form a magnified image of the sample (21), **characterized in that** the light collecting side condenser lens (25) is a long focal distance lens, and a light shielding member (23) for shielding the illumination light (11) is provided at an image forming center of a back focal plane in the image forming optical system.
2. A dark field microscope comprising a light source for emitting illumination light (10, 11) a light collecting optical system including a light collecting side condenser lens (25) for collecting the illumination light (10) from the light source to illuminate an observation sample (21), an image forming optical system including an objective lens (22) for receiving scattered light (12) from the observation sample (21) to form a magnified image of the sample (21), **characterized in that** the light collecting side condenser lens (25) is a long focal distance lens, and a light shielding member (23) for shielding the illumination light (11) is provided at an image forming center of a conjugate image of a back focal plane in the image forming optical system.
3. The dark field microscope according to claim 2, **characterized in that** a lens for forming a secondary image from a primary image, and forming the conjugate image of the back focal plane between them is disposed in the image forming optical system.
4. The dark field microscope according to claim 3, **characterized in that** the light shielding member (23) disposed at the image forming center of the conjugate image of the back focal plane is a light shielding plate having a diameter of $\phi_e = \phi \cdot f_1 / L$ (ϕ is a diameter of an area to be shielded on the back focal plane; f_1 is a focal distance of the lens for forming the conjugate image of the back focal plane; and L is a focal distance of a second objective lens).
5. The dark field microscope according to claim 3, **characterized in that** the image forming optical system for forming the secondary image from the primary image comprises a plurality of lenses, and a total focal distance of lenses for forming the conjugate image of the back focal plane among the plurality of lenses is $f_t = L \cdot \phi_e / \phi$ (L is a focal distance of a second objective lens; ϕ_e is a diameter of the light shielding member (23) and ϕ is a diameter of an area to be shielded on the back focal plane).

6. The dark field microscope according to anyone of claims 1 to 5, comprising a mirror between the primary image and the secondary image.

5 7. A dark field microscope adjusting method wherein, in a configuration comprising the dark field microscope according to any of claims 1 to 6 and a camera for receiving an image by the dark field microscope, an optical axis adjustment is performed by :

10 adjusting a focal point of an eyepiece lens to focus on the observation sample (21) ;
adjusting a position of the light collection side condenser lens (25) to thereby provide Koehler illumination ;
adjusting a position of the image forming side lens to thereby focus the observation sample (21) on the imaging area;
adjusting a diaphragm for a primary imaging plane and a position of the mirror to thereby match a field center with a center of the camera; and
15 adjusting a position of the light shielding member (23) in an optical axis direction to set it at a position where background light is reduced to a minimum.

8. The dark field microscope adjusting method according to claim 7, **characterized in that** the position of the light shielding member (23) is adjusted in a direction which is perpendicular to the optical axis.

20 9. The dark field microscope adjusting method according to claim 7 or 8, comprising :

minimizing a field diaphragm on the light collecting side condenser lens,
adjusting a black level with preventing the light from entering the camera, to thereby set a value of the level not to take a negative value,
25 switching the light to a camera side and adjusting an aperture diaphragm with the observation sample being focused on, to thereby set the aperture diaphragm at a position where the image darkens, and
adjusting the light intensity and the aperture diaphragm to thereby increase an amount of light and narrow a numerical aperture.

30 10. The dark field microscope adjusting method according to any of claims 7 to 9, comprising adjusting the black level to thereby optimize a background of the observation sample (21).

35 11. The dark field microscope adjusting method according to any of claims 7 to 10, comprising adjusting the light intensity to thereby increase scattered light (12) from the observation sample (21).

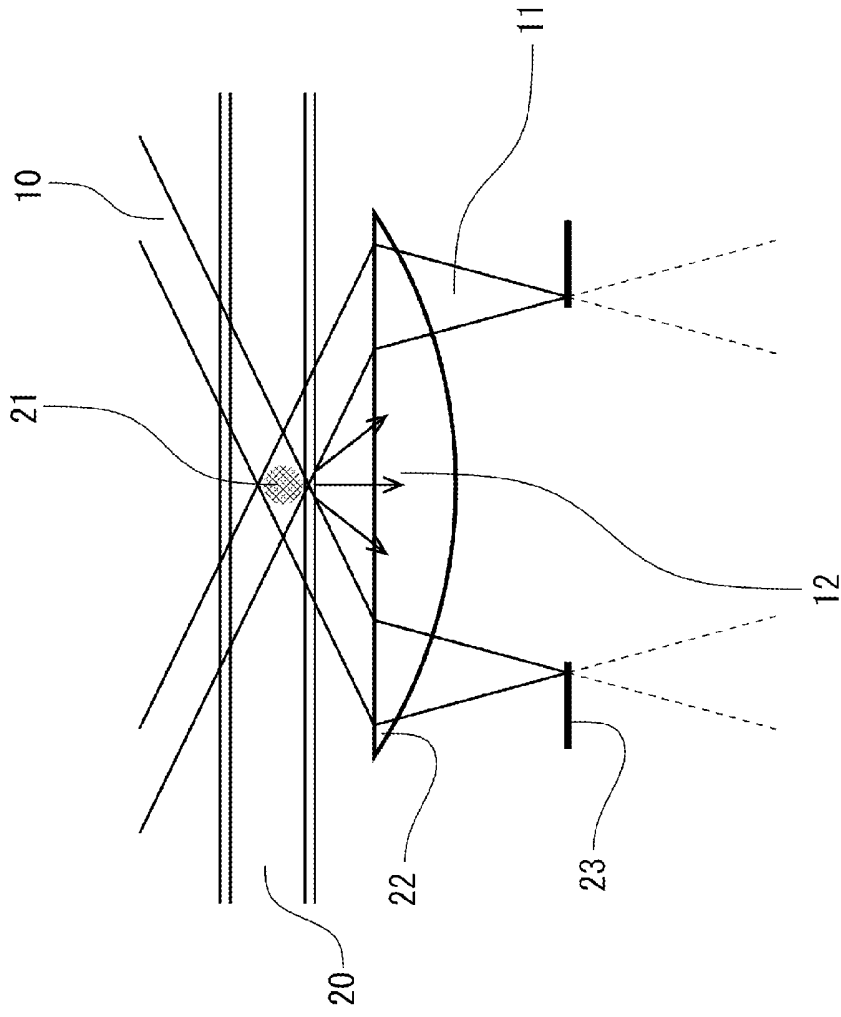


Fig. 1

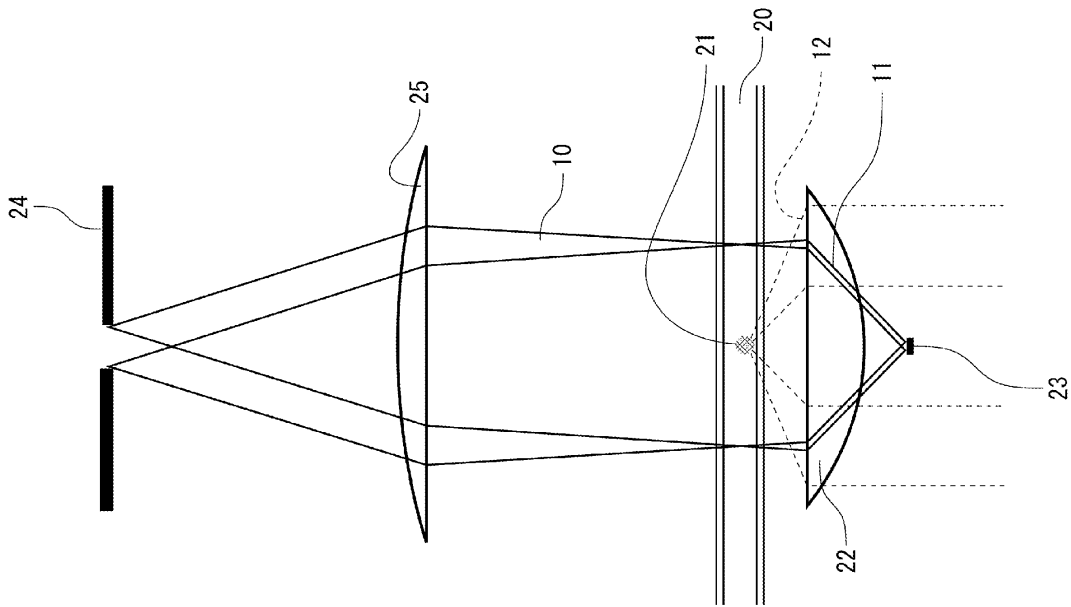


Fig. 2

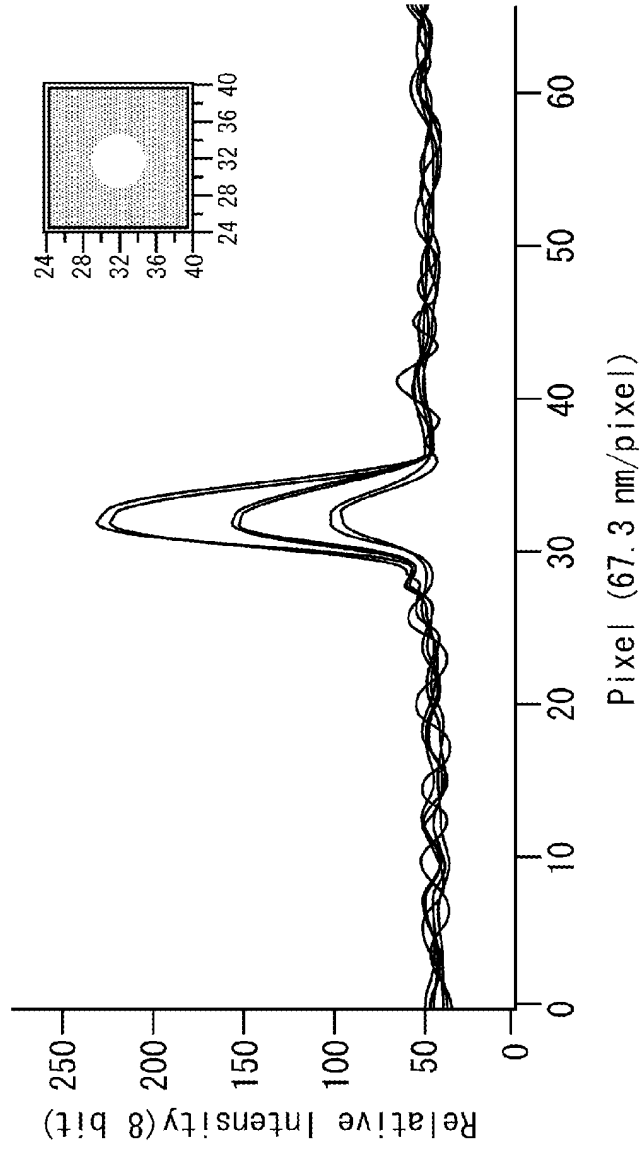


Fig. 3

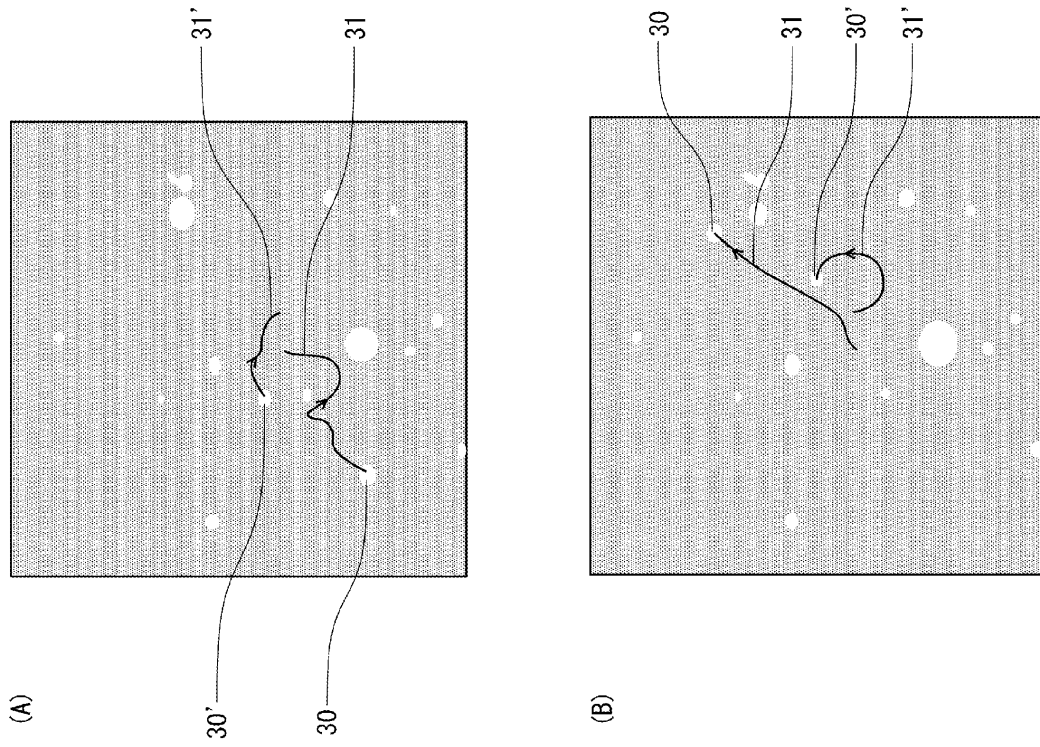


Fig. 4

INTERNATIONAL SEARCH REPORT

International application No.

PCT/JP2007/060554

A. CLASSIFICATION OF SUBJECT MATTER

G02B21/00 (2006.01) i

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

G02B21/00

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Jitsuyo Shinan Koho 1922-1996 Jitsuyo Shinan Toroku Koho 1996-2007

Kokai Jitsuyo Shinan Koho 1971-2007 Toroku Jitsuyo Shinan Koho 1994-2007

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	JP 7-5397 A (Canon Inc.), 10 January, 1995 (10.01.95), Page 3, left column, line 4 to right column, line 11; Fig. 1 (Family: none)	1-11
X A	JP 2002-221666 A (Sumitomo Chemical Co., Ltd.), 09 August, 2002 (09.08.02), Par. No. [0007]; Fig. 1 (Family: none)	1-6 7-11

 Further documents are listed in the continuation of Box C. See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search
20 August, 2007 (20.08.07)Date of mailing of the international search report
28 August, 2007 (28.08.07)Name and mailing address of the ISA/
Japanese Patent Office

Authorized officer

Facsimile No.

Telephone No.

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP H09297266 B [0007]
- JP H0915507 B [0007]
- JP H08122651 B [0007]
- JP H05346532 B [0007]

Non-patent literature cited in the description

- **YASUDA, R. ; NOJI, H. ; YOSHIDA, M. ; KINOSITA, K., JR. ; ITOH, H.** Resolution of distinct rotational substeps by submillisecond kinetic analysis of F1-ATPase. *Nature*, 2001, vol. 410, 898-904 [0050]